

© Copyright 2010, Brooks Instrument, LLC All rights reserved. Printed in USA









Variable Area, High Flow Glass Tube

High Flow Glass Tube Variable Area **Flow Meters**

Quick Start Guide

Read this page before proceeding!

MARNING

- Read all instructions prior to installing, operating and servicing this product.
- this product. Follow all warnings, cautions and instructions marked on and supplied with
- Failure to heed this warning can result in serious personal injury and/or damage Do not operate this equipment in excess of the specifications listed on the meter.
- If the inlet and outlet valves adjacent to the flowmeter are to be closed for any ro rue eduibment.
- possible personal injury. thermal expansion of the liquid which can cause rupture of the meter and reason, the flowmeter must be completely drained. Failure to do so may result in
- Failure to correctly purge the meter could result in fire, explosion or death. dry, inert gas such as nitrogen before disconnecting the gas connections. toxic, pyrophoric, flammable or corrosive gas, purge the meter thoroughly with a

excessive pressure or flow surges. Protective devices should be installed upstream from this instrument, such as flow controllers, pressure regulators,

static electricity. Proper handling procedures must be observed during the If this instrument contains electronic components it is susceptible to damage by

instruction manual for proper wiring. If this instrument contains electronic components consult the complete

Z

Brooks Instrument 1-4-4 Kitasuna Koto Ku Tokyo, 136-0073 Japan Tel +81 (0) 3 5633 7100 Fax +81 (0) 3 5633 7101

E-mail BrooksAs@BrooksInstrument.com

Brooks is a trademark of Brooks Instrument, LLC

E-mail BrooksEu@BrooksInstrument.com

Brooks Instrument Neonstraat 3 6718 WX Ede, Netherlands P.O. Box 428

6710 BK Ede, Netherlands Tel +31 (0) 318 549 300 Fax +31 (0) 318 549 309

Hatfield, PA 19440-0903 USA Tel (215) 362 3700 Fax (215) 362 3745

P.O.Box 903 E-mail BrooksAm@BrooksInstrument.com

407 West Vine Street

Brooks Instrument

Visit us online at www.BrooksInstrument.com

Dear Customer,

that matters - real users of flow instrumentation, like you. category for accuracy, reliability and user preference, as judged by the audience award-winning meters and controllers consistently rank at the top of their measurement and control needs with a Brooks Instrument device. Brooks' Thank you for your purchase. We appreciate this opportunity to service your flow

local Brooks product and application specialist is truly your "partner in flow". unsurpassed local technical expertise in virtually every corner of the planet. Your But Brooks' products are only half of the story. You are backed by Brooks'

application problems just like yours. your flow measurement or control needs and offer years of experience solving They have been extensively trained to help you select the optimal solutions for

back cover of this guide. services, please contact your local Brooks Sales and Service office listed on the Should you require any additional information concerning Brooks' products and


Brooks Instrument Sincerely,

This Quick Start Guide applies to the following Brooks product(s):

- GT1000 Series (Full-View)
- CLJJ00
- · 011305, 611306, 611307 · CIJ303

instruction manuals with product shipments to reduce our paper consumption. In an effort to be more eco-friendly, Brooks is no longer supplying printed

"(staters, High Flow Glass Tube (Rotameters)" Area and click on "Variable Area www.BrooksInstruments. For these product's complete instruction manual, please download it at

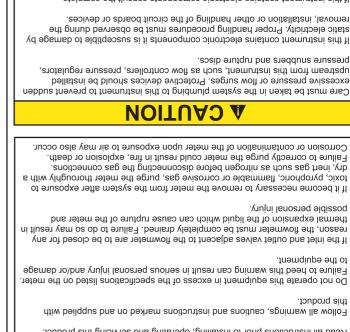



Installation (See Figures 1 and 2)

- a. Carefully remove the covers from each end of the flowmeter.
- b. Install the flowmeter with the inlet at the bottom and the outlet at the top.
- c. When installing the flowmeter in the process line, follow accepted plumbing practices for flanged or threaded fittings.
- d. Install the flowmeter within 5° of true vertical. Use of a level is recommended to determine the proper alignment.
- e. Installation of a bypass piping arrangement is recommended, see Figures 1 and 2 Typical Flowmeter Installations. Bypass piping permits the meter to be isolated from the flow for servicing and cleaning.

Pressure Equipment Directive (97/23/EC)

Note: Equipment falls under Sound Engineering Practice (SEP) according to the directive.

It is recommended that a final leak test of the system plumbing and the meter be performed before subjecting it to the process fluid.

NOTE: If the device includes an Alarm, please reference the complete instruction manual for proper installation instructions.

Installation

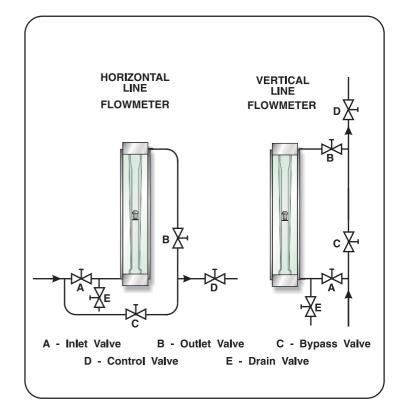


Figure 1 Typical Flowmeter Installation

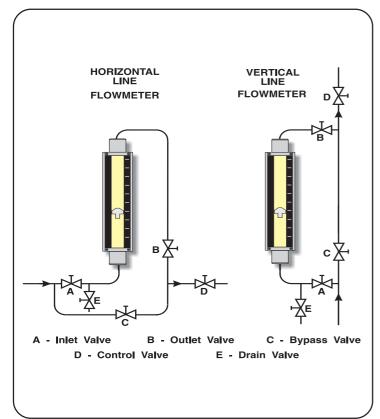


Figure 2 Typical Flowmeter Installation

Operation

After the flowmeter has been installed in the flow system, it is ready for operation. An optional built-in needle control valve may be provided to control the flow through the flowmeter. These control valves are designed for control. Excessive tightening may damage the valve seat and limit its effectiveness as a control valve. If tight shut-off is required, it is recommended that a separate shut-off valve is installed in the process line immediately before the flowmeter.

Equipment Receipt and Return Procedures

Receipt of Equipment

If the packing case is damaged, the local carrier should be notified at once regarding their liability. Carefully remove the equipment from the packing case and inspect for damage or missing parts. If damaged, please contact Brooks Instrument at one of the locations listed on the back of this Quick Start Guide.

Return Shipment

Please note that prior to returning any instrument to the factory Brooks Instrument requires the completion of Form RPR003-1, a Brooks Instrument Decontamination Statement, as well as a Materials Safety Data Sheet (MSDS) for fluid(s) used in the instrument. Copies of these forms can be found online at **BrooksInstrument.com/Returns** along with complete details on how to process your return shipment or you can contact your nearest Brooks location for the necessary forms and instruction.

Δ

5